



DEVICE CONNECTIVITY FOR
POINT-OF-CARE TESTING

RALS™ DEVICE INTERFACING

Helena Actalyke Activated Clotting Time analyzers are designed for the management of heparin anticoagulation at the point of care.

CONNECTIVITY TO RALS ENABLES USERS TO:


- Centralize all test results into the RALS system
- Transfer results to an EMR/EHR/LIS
- Email results to operators and managers
- Access and manage mis-identified patient and out of range QC results



VISIT RALS.COM

RALS™ | Helena Actalyke Analyzer Interfacing

HOSPITAL / FACILITY / INSTITUTION NETWORK

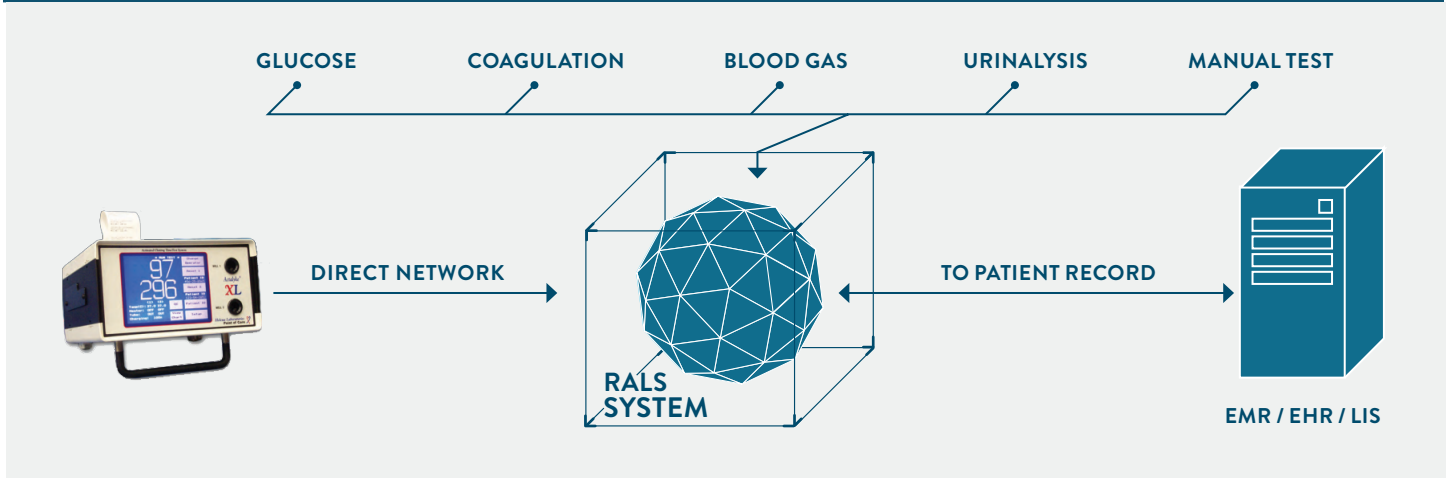

DATA FLOW

Helena Actalyke analyzers transfer data to RALS via a direct network connection where it is evaluated and either sent directly to the EMR/EHR/LIS or held for review.

UNI-DIRECTIONAL COMMUNICATION

Data sent from the device to RALS

- Results (Patient, QC, EQC)
- Patient ID
- Operator ID
- Date/Time
- Location

AVAILABLE REPORTS FROM THE RALS SYSTEM

- RALS Devices Log
- Workload Summary
- Anomalous Results by Device
- Anomalous Results by Operator
- Operator Pending Recertification Range
- Operator Pending Recertification Date
- Operators with No Certifications
- Operator Statistics
- Patient Results by Operator
- Patient Results by Patient
- LIS Statistics by Location
- LIS Statistics by Operator
- Institution Statistics
- Location Statistics
- Levey-Jennings
- QC Test Results
- Device Statistics Summary
- Test Materials

TO LEARN MORE, VISIT RALS.COM

© 2019 Abbott. All rights reserved. All trademarks referenced are trademarks of either the Abbott group of companies or their respective owners. Any photos displayed are for illustrative purposes only. Any person depicted in such photos is a model. AI-COLL-0119 Rev. 1 12/19

