




DEVICE CONNECTIVITY FOR
POINT-OF-CARE TESTING

RALS™ DEVICE INTERFACING

The BD Veritor™ Plus System provides lab-quality immunoassay test results and can help detect infectious diseases such as influenza A and B, respiratory syncytial virus (RSV) and group A strep.

CONNECTIVITY BY THE RALS™ SYSTEM ENABLES USERS TO:


- Centralize all POC test results into the RALS System
- Transfer results to any EMR/EHR/LIS
- Email results to operators and managers
- Access and manage misidentified patient and out-of-range QC results
- Monitor and manage operator certifications

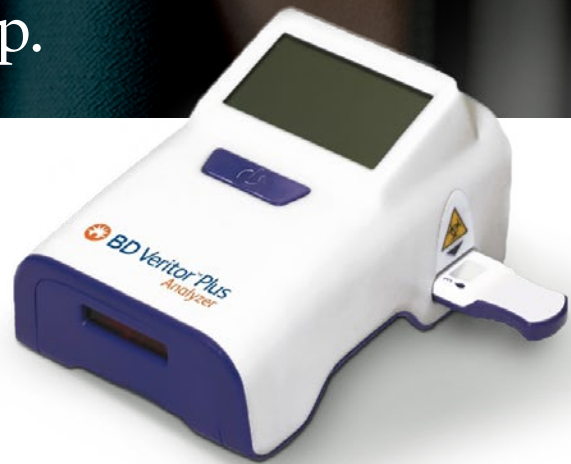

VISIT RALS.COM

RALS™ | BD Veritor™ Plus System Connectivity

HOSPITAL / FACILITY / INSTITUTION NETWORK

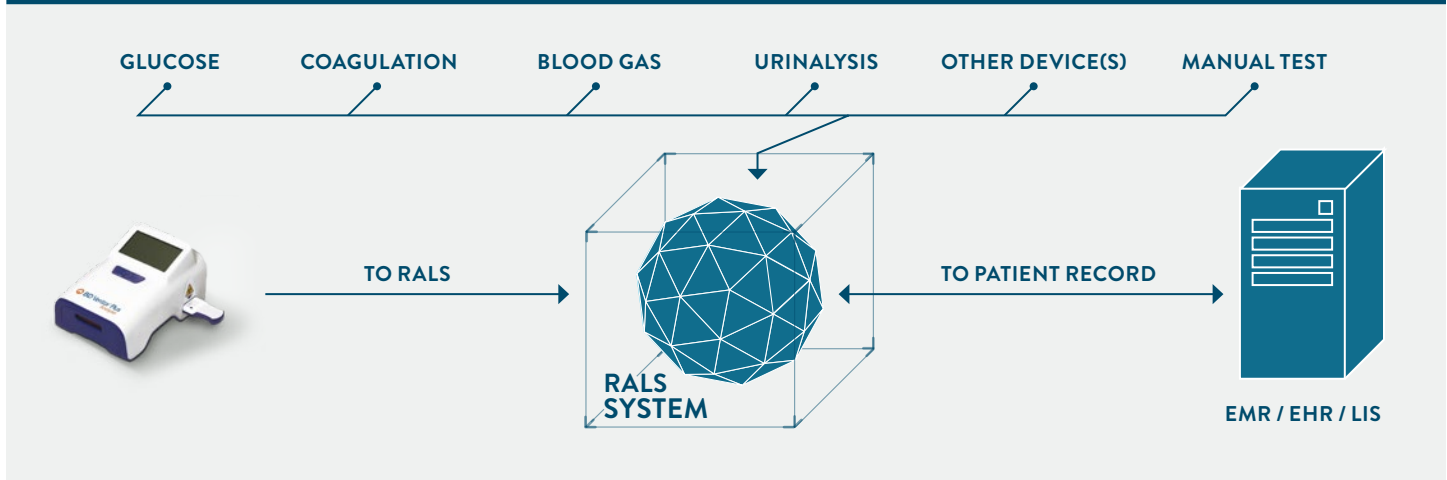

TYPE OF TESTS PERFORMED

The BD Veritor Plus System performs the following CLIA-waived tests:

- Flu A+B
- RSV
- Strep

UNI-DIRECTIONAL COMMUNICATION

From device to RALS System:

- Patient test results
- QC test results
- Operator ID
- Date/time
- Materials

How the device connects:

- The device communicates with RALS via the BD Cloud Connectivity Solution

AVAILABLE REPORTS

- Anomalous Results by Device
- Anomalous Results by Operator
- Institution Statistics
- LIS Statistics by Location
- LIS Statistics by Operator
- Operator ID Compliance by Location
- Operator Pending Recertification Date
- Operator Statistics
- Operator Proficiency
- Patient ID Compliance by Operator
- Patient ID Compliance by Location
- Patient Results by Location
- Patient Results by Operator
- Patient Results by Patient
- QC Test Results
- Device Statistics Summary
- Test Materials
- Workload Summary

TO LEARN MORE, VISIT [RALS.COM](https://www.rals.com)

© 2019 Abbott. All rights reserved. All trademarks referenced are trademarks of either the Abbott group of companies or their respective owners. Any photos displayed are for illustrative purposes only. Any person depicted in such photos is a model. INFO272667 AI-COLL-0117 Rev. 1 12/19

