



DEVICE CONNECTIVITY FOR POINT-OF-CARE TESTING

RALS™ DEVICE INTERFACING

Designed to meet the challenges of point-of-care settings, Siemens RAPIDPoint® Blood Gas Systems, which include RAPIDPoint 400, 405 and 500 analyzers, deliver fast, accurate and comprehensive test results.

CONNECTIVITY BY THE RALS™ SYSTEM ENABLES USERS TO:


- Centralize all point-of-care test results into the RALS system
- Transfer results to any EMR/EHR/LIS
- Email results to operators and managers
- Access and manage misidentified patient and out-of-range quality control (QC) results
- Monitor and manage operator certifications



VISIT RALS.COM

RALS™ | RAPIDPoint® Blood Gas System Connectivity

HOSPITAL/FACILITY/INSTITUTION NETWORK

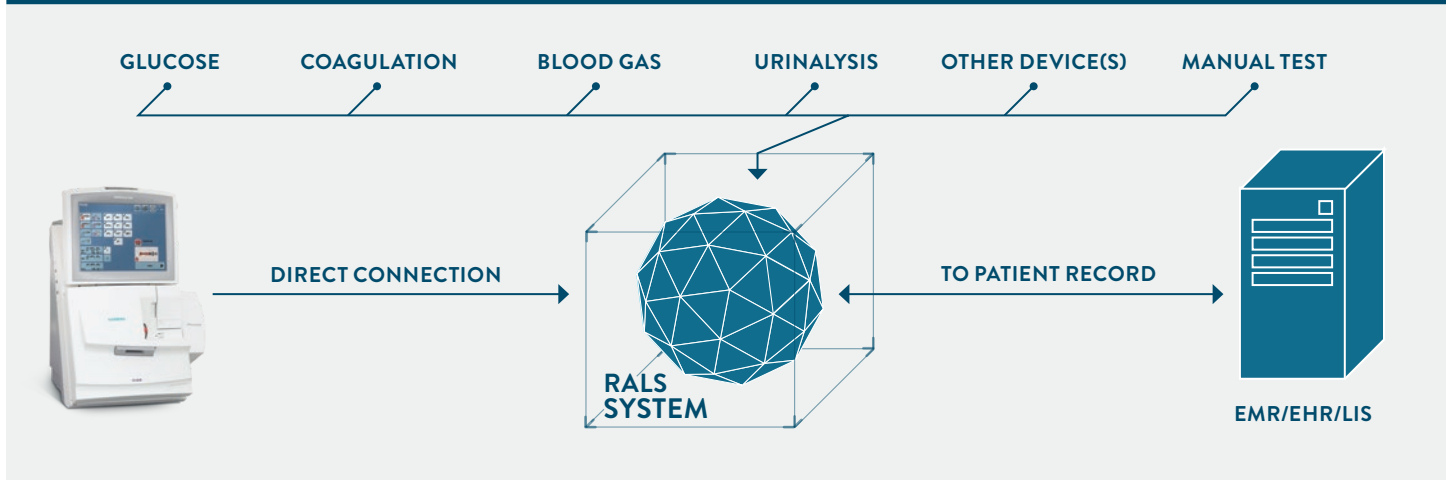

DATA FLOW

RAPIDPoint® analyzers transfer data to RALS™ via a TCP/IP connection where it is evaluated and either sent directly to the EMR/EHR/LIS or held for review.

UNI-DIRECTIONAL COMMUNICATION

From Device to RALS:

- Patient, QC and calibration results

How the Device Connects:

- Direct Ethernet connection

AVAILABLE REPORTS

- Anomalous Results by Device
- Anomalous Results by Operator
- Institution Statistics
- Location Statistics
- LIS Statistics by Location
- LIS Statistics by Operator
- Operator ID Compliance by Location
- Operator Pending
- Recertification Date
- Operator Pending
- Recertification Range
- Operator Statistics
- Patient ID Compliance by Operator
- Patient ID Compliance by Location
- Patient Results by Operator
- Patient Results by Patient
- QC Test Results
- Device Statistics Summary
- Corrective Action Compliance by Location and by Operator
- Patient Result Comments
- Comment Codes
- Test Materials
- Workload Summary
- Operators with No Certifications
- RALS Device Log

TO LEARN MORE, VISIT RALS.COM

© 2019 Abbott. All rights reserved. All trademarks referenced are trademarks of either the Abbott group of companies or their respective owners. Any photos displayed are for illustrative purposes only. AI-COLL-0131 Rev 1 12/19

